



POLISH CENTRE FOR TESTING AND CERTIFICATION

02-699 Warszawa, ul. Kłobucka 23A

Mechanical Laboratory

tel.: (+48 22) 46 45 594; fax: (+48 22) 46 45 563

e-mail: labmech@pcbc.gov.pl

Date: 12.04.2010

TEST REPORT NO. BR – 055/L-071/2010

Page 1 of 4

Subject of testing: *Shower Chair with tilt*

Classification according to PN-EN ISO 9999:2001 :
09 33 03

Type/Model 302024

Catalogue no.: ---

Manufacturer : *MOBILEX A/S, Noerskovvej 1
DK - 8660 Skanderborg*

Number of specimens : 1

Applicant: *A-Net s.c. 93-469 Łódź,
ul. Łaskowice174*

Kind of testing *Testing scope according to application of Client
Mechanical testing for conformity with PN-EN 12182:2005
excluding clause 4.1, 4.3, 5.2, 22, 24*

Test started: 6.04.2010

Test finished : 12.04.2010

Performed by:

Checked by :

Approved by :

Mirosław Szymański

Ireneusz Czerwiński

KIEROWNIK
LABORATORIUM MECHANICZNEGO

mgr inż. Andrzej Tkaczyk

Special comments / enclosures:

Copyright © 2005 by Polish Centre for Testing and Certification (applicable to report form)

Test results refer only to tested units.

Test results reported here are not applicable to the further modifications of the product affecting its structure, material or technology.

This test report shall be neither copied differently as in the whole nor be published without written consent of the Laboratory.




TESTING

NORMATIVE REFERENCES

PN-EN 12182:2005

Technical aids for disabled persons – General requirements and test methods

PHOTO OF PRODUCT

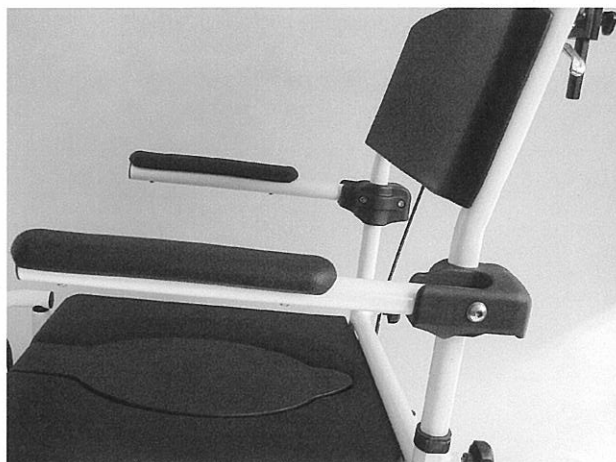

MOBILEX A/S
Noerskovvej 1
DK - 8660 Skanderborg
Tel: +45 87 93 22 20
www.mobilex-care.com

Shower chair
with tilt



Max. 130 kg



Warning!
Be Careful!
Risk of finger cut!

CE Produced Serial no.

CHARAKTERISTICS OF PRODUCT

Name of product: Shower Chair with tilt Maximum weight of user: 130 kg Mass of product: 15,1 kg

Dimensions:

Overall height with headrest:	970 mm – 1410 mm
Overall height without headrest:	850 mm – 1110 mm
Maximum width:	558 mm
Maximum length (max. moving of footrest and headrest):	1310 mm
Minimum length(min. moving of footrest and headrest):	860 mm
Height of seat:	585 mm/535 mm (2 levels of adjustment)
Angle of seat plane:	from - 6,5° to + 25,5°

Material:

Aluminum alloy, plastic



TEST RESULTS according to PN-EN 12182 : 2005

Requirements according to clause	Test method according to clause	Checked characteristics/assemblies/parameters		Real value	Test result	Comments
4.1	5.2, 5.4.2, 5.5, 6, 8.2.1, 9.4, 10, 22, 24 i EN 1441	Risk analysis		-	N/T	
4.2	V/I	Expected characteristics and technical documentation		Conf.	Pos.	
4.3	EN-540	Clinic assessment		-	N/T	
4.4	V/I	Technical support which can be dismantled		Conf.	Pos.	
4.5	V/I	Single use connections		Conf.	Pos.	
4.6	V/I	Boundary values of user weight		Conf.	Pos.	
5.1	V/I	Flammability		-	N/A	
5.2	EN ISO 10993-1	Biological conformity and toxicity		-	N/T	
5.3	V/I	Impurities and residues		-	N/A	
5.4	24, Annex.C C.5.4.1	Microbiological infections and contamination	Cleaning	Conf.	Pos.	
	24, Annex.C C.5.4.1		Disinfection	-	N/A	
	EN 12442-1		Animal tissue	-	N/A	
6	Measur.	Noise		-	N/A	
7	Measur.	Electromagnetic compatibility		-	N/A	
8	EN60601-1 EN60335-1	Electrical safety		-	N/A	
9	V/I	Overflowing, pouring out, leakage and pouring in of liquids		-	N/A	
10	V/I. Measur.	Surface temperature		-	N/A	
11	V/I	Sterility		-	N/A	
12	V/I. Measur.	Safety of moving elements		Conf.	Pos.	Warnings in service manual
13	V/I. Measur.	Trap prevention for parts of human body		Conf.	Pos.	
14	V/I. Measur.	Folding and adjusting of mechanisms		Conf.	Pos.	
15	V/I. Measur.	Hand grips for transferring		--	N/A	
16	V/I. Measur.	Aids for support of users		Conf.	Pos.	
17	V/I	Portable and moving technical aids		-	N/A	
18	V/I	Surfaces, corners and edges		Conf.	Pos.	
19	Annex.C,C18	Hand kept technical aids		-	N/A	
20	V/I	Grips and other elements for transferring		-	N/A	Mass of product below 20 kg
21	V/I	Force action on soft tissues of human body		Conf.	Pos.	
22	Annex.C22	Ergonomic principles – action force		-	N/T	The requirements relate to the design process
23	V/I	Information provided by manufacturer		Conf.	Pos.	
24	V/I	Package		-	N/T	Note 1

Pos. – positive; Neg – negative; N/T – not tested; N/A – not applicable; N/R – not required, N/O – not occurred, V/I.- visual inspection, Conf.- conformed.

NOTE 1: Assessment of package , clause 24 concerns risk of threats caused by improper protection against damage, fall or impurity during storage and transport to place of use

NOTE 2. Risk analysis performed by the manufacturer should take into account requirements of PN-EN 12182:2005 clause 5.2, 5.4.2, 5.5, 6, 8.2.1, 9.4, 10, 22 i 24

NOTE 3. Conformity assessment of product according to standard requirements refer to the scope of mechanical tests ordered by client

CONCLUSIONS:

*Testing object **conforming** with requirements of PN-EN 12182 :2005, excluding clause 4.1, 4.3, 5.2, 22, 24*

----END----